

# 3D Localizers for Surgical Navigation


## 600.455/655

Russell H. Taylor




1


## Traditional Stereotactic Systems



Cosman-Roberts-Wells (CRW) head frame



CT Image




Brown-Roberts-Wells (BRW) head frame



2

## Surgical Navigation Systems

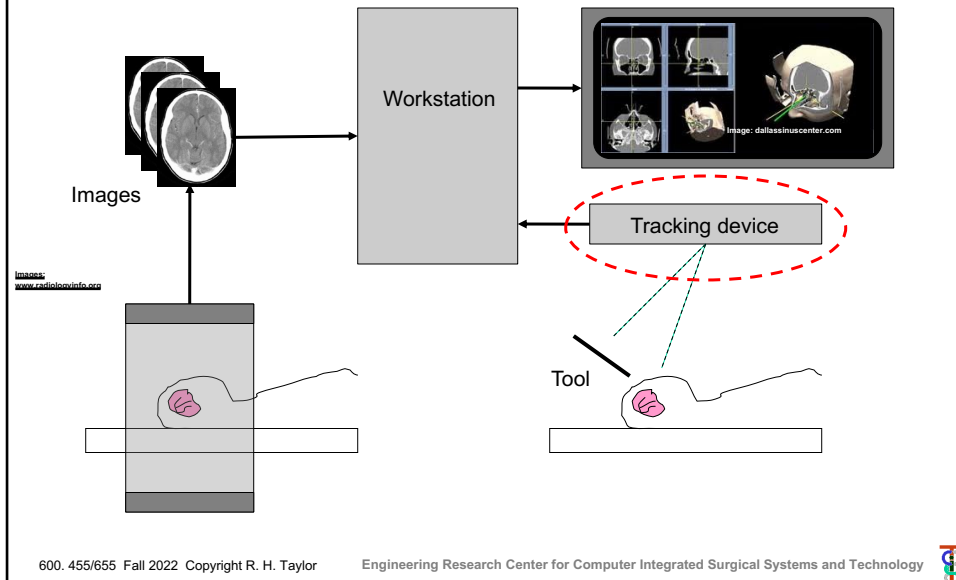

3

## 3D localizers

- Determine 3D positions in space relative to some coordinate system
- Also called “3D digitizers”, “3D navigation systems”, “localizers”, etc.
- Many uses
- Many technologies

600. 455/655 Fall 2022 Copyright R. H. Taylor Engineering Research Center for Computer Integrated Surgical Systems and Technology

4

## Localizer technologies

- Instrumented passive manipulator
- Active manipulator
- Ultrasound
- Electromagnetic
- Optical active
- Optical passive
- Miscellaneous – e.g., fiber optic


Engineering Research Center for Computer Integrated Surgical Systems and Technology



5

## Passive mechanical linkages

- Encoders & linkage

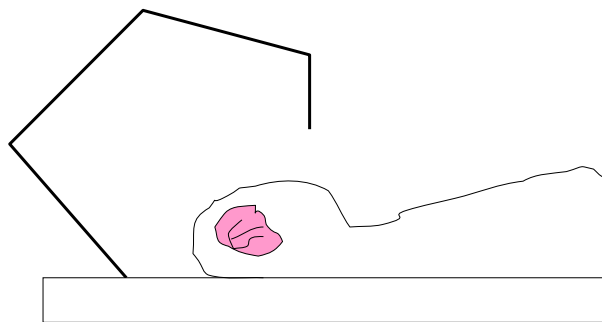


600. 455/655 Fall 2022 Copyright R. H. Taylor

Engineering Research Center for Computer Integrated Surgical Systems and Technology




6

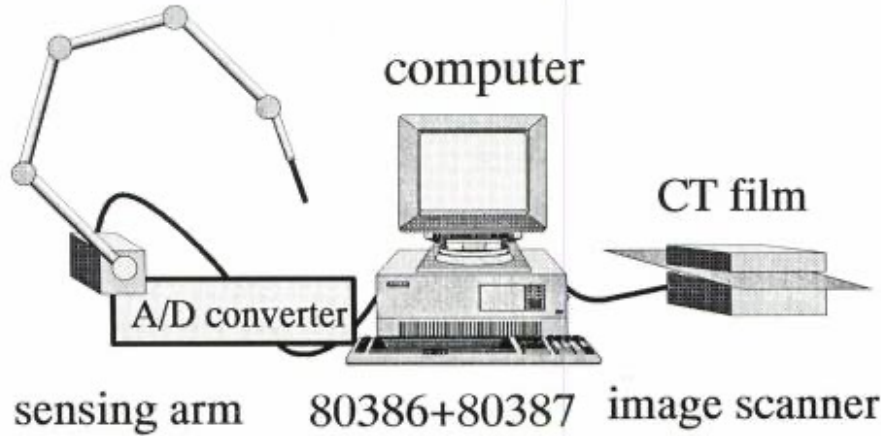

*Figure 1. A schematic representation of the neuronavigator system. It consists of a microprocessor and a multi-articulated arm structure.*




7

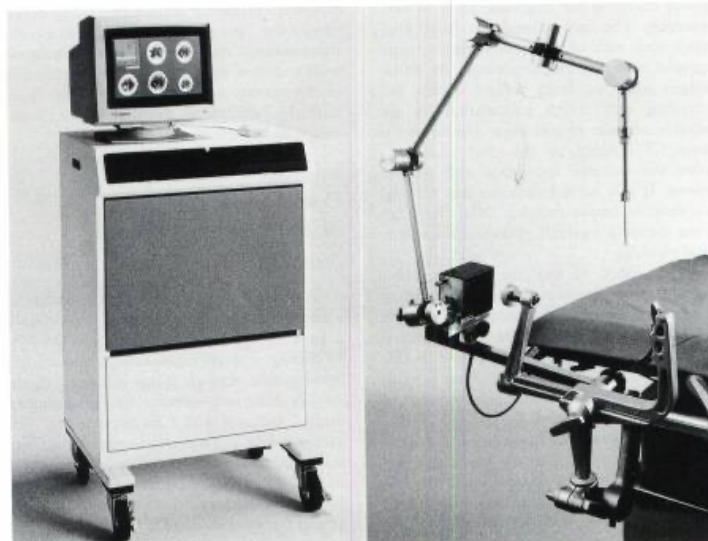


*Figure 2. Photograph of the neuronavigator. The computer system is housed in the console box on the left. The sensing arm is secured to the Mayfield skull clamp. Six CT slices are displayed on the computer screen. Two cross markers display the location of the navigator tip.*




8

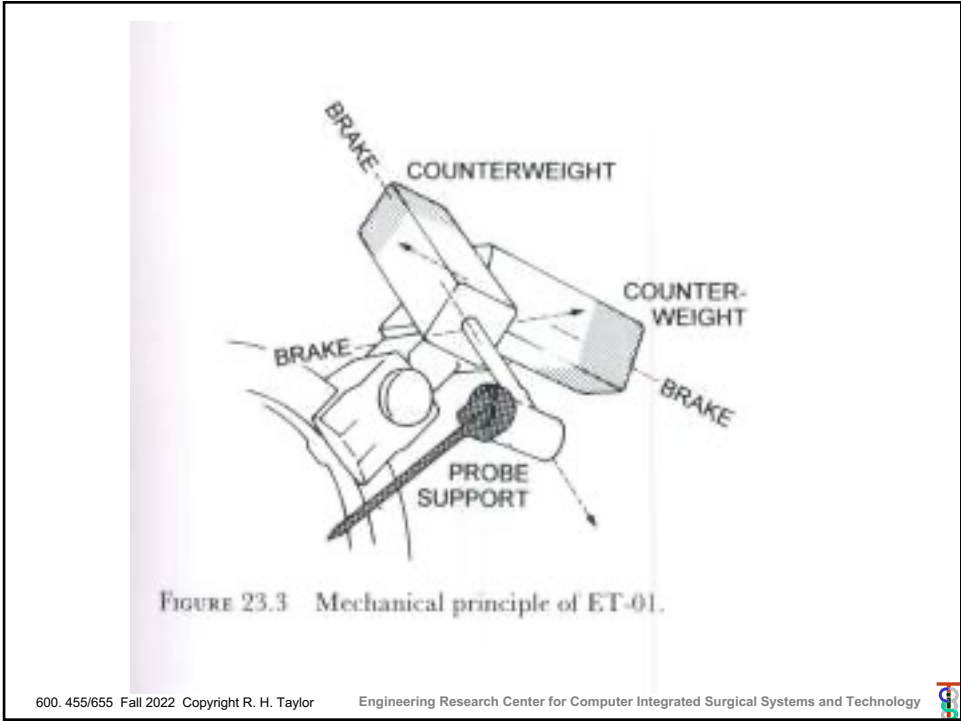


9

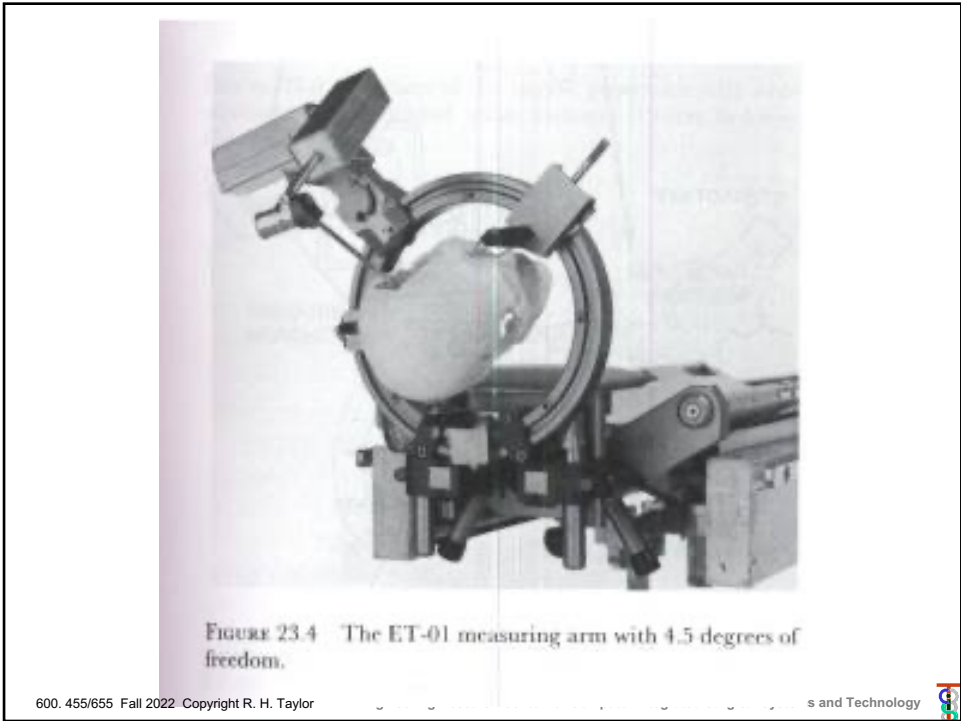

10

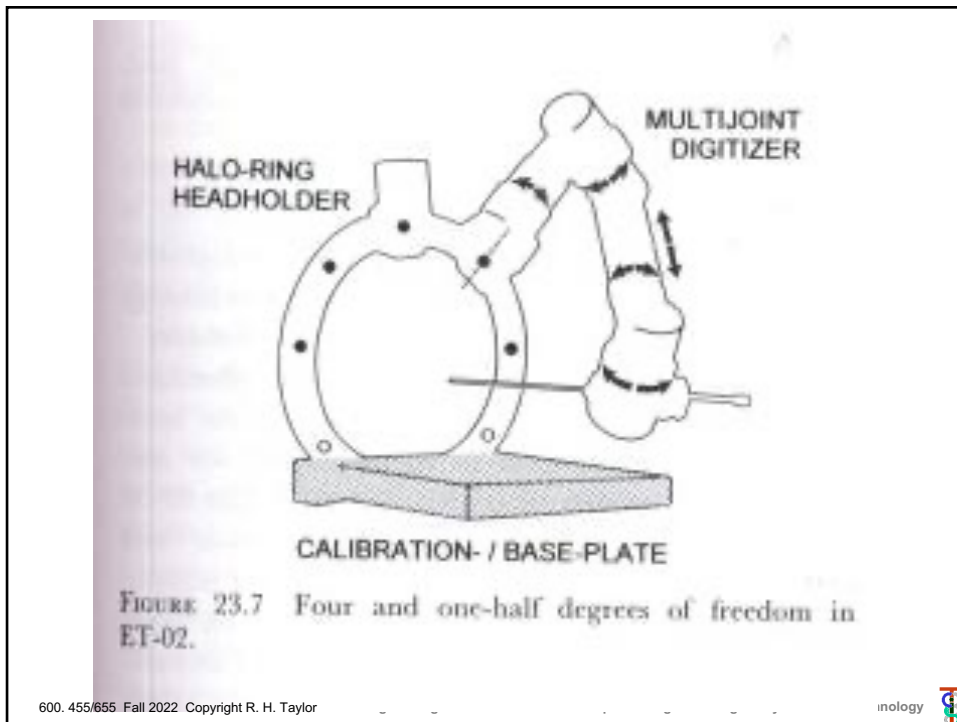

11

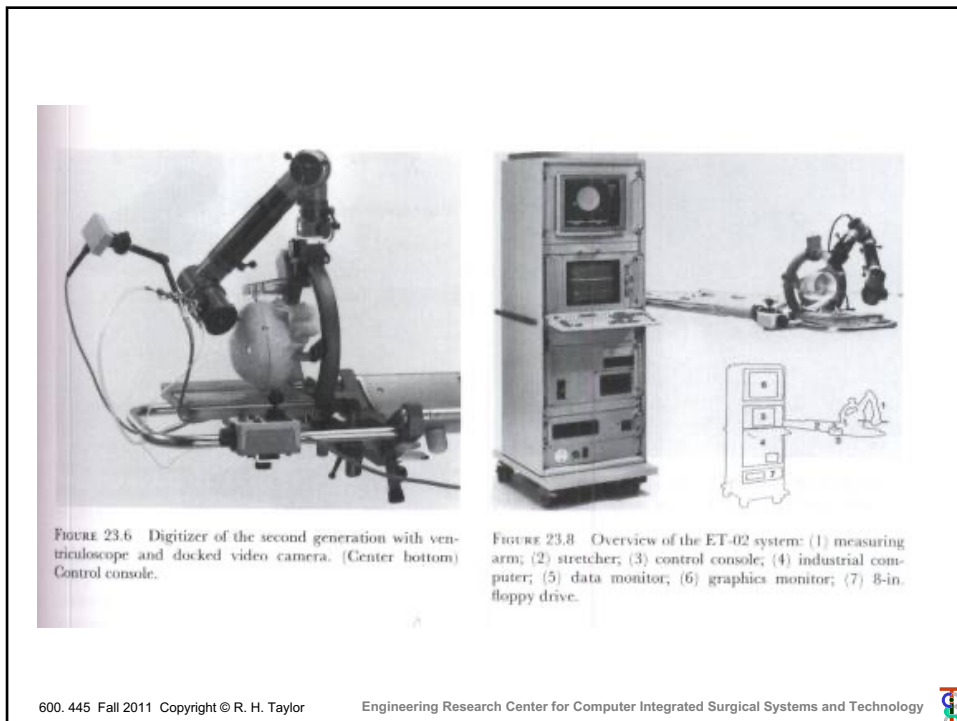

12

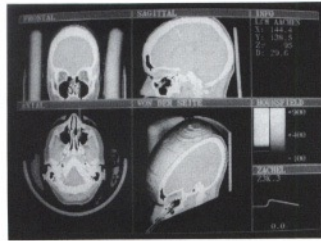



FIGURE 51.1 Image display on the CAS monitor screen.


Therefore, we developed an appropriate measuring device which has 6 degrees of freedom [2, 3]. Digital increment encoders have been applied for shaft angle measurement. The pulse signals of the six rotary encoders are evaluated by 16-bit counters. A dedicated 68008 microcomputer calculates the position of the measuring probe from the measured angles and the given arm lengths. The system was developed with 3D imaging (figure 51.1).

A third generation of mechanical systems was developed to achieve better intraoperative handling [4] (figure 51.2). Counterbalanced arm elements allow for easy movements in every position. The 68008 was replaced by a PC-486.



FIGURE 51.2 The Aachen device for CAS with electro-mechanical measuring arm (coordinate digitizer).


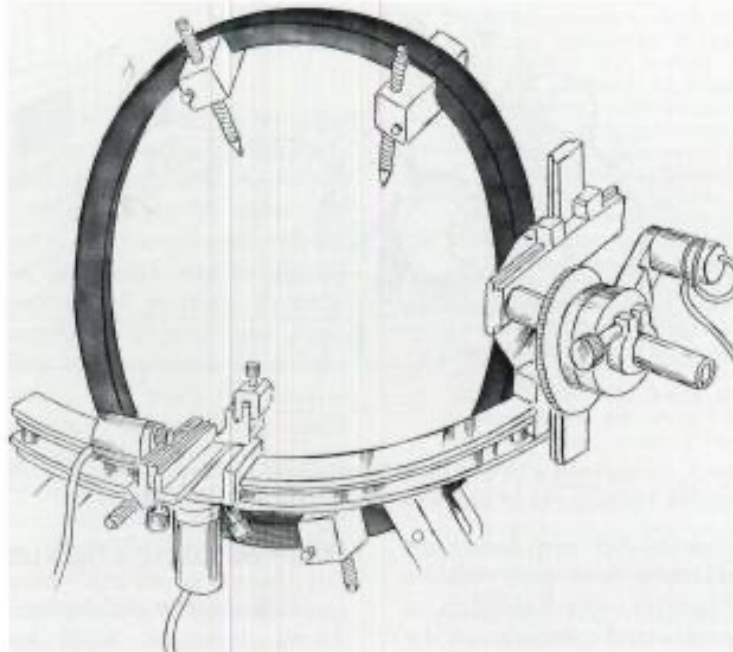


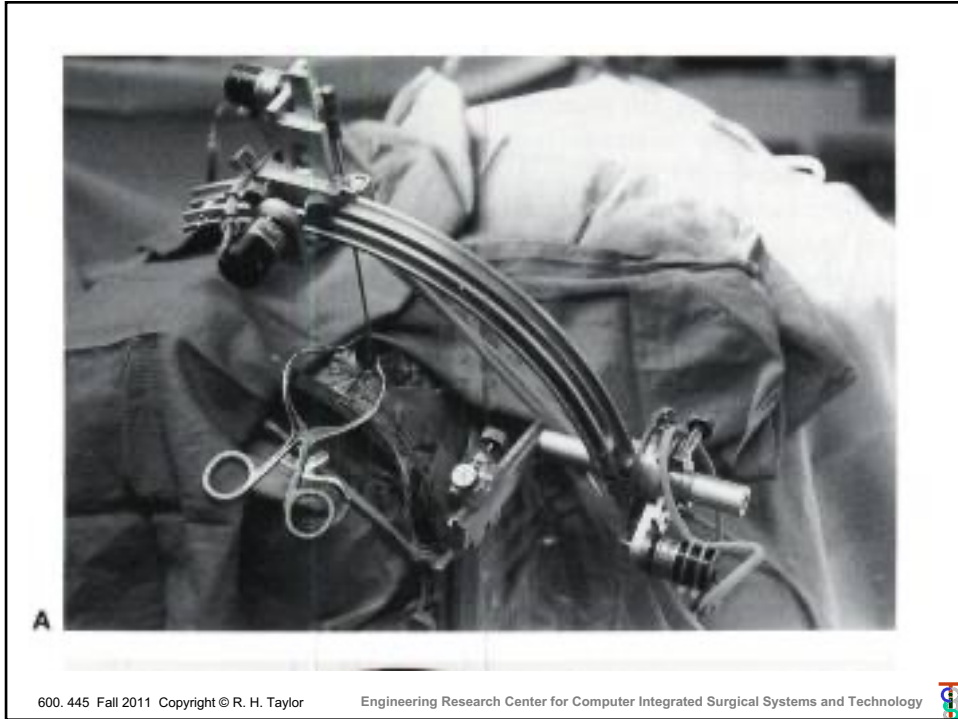

15

## Passive mechanical linkages

- Encoders & linkage
- Advantages

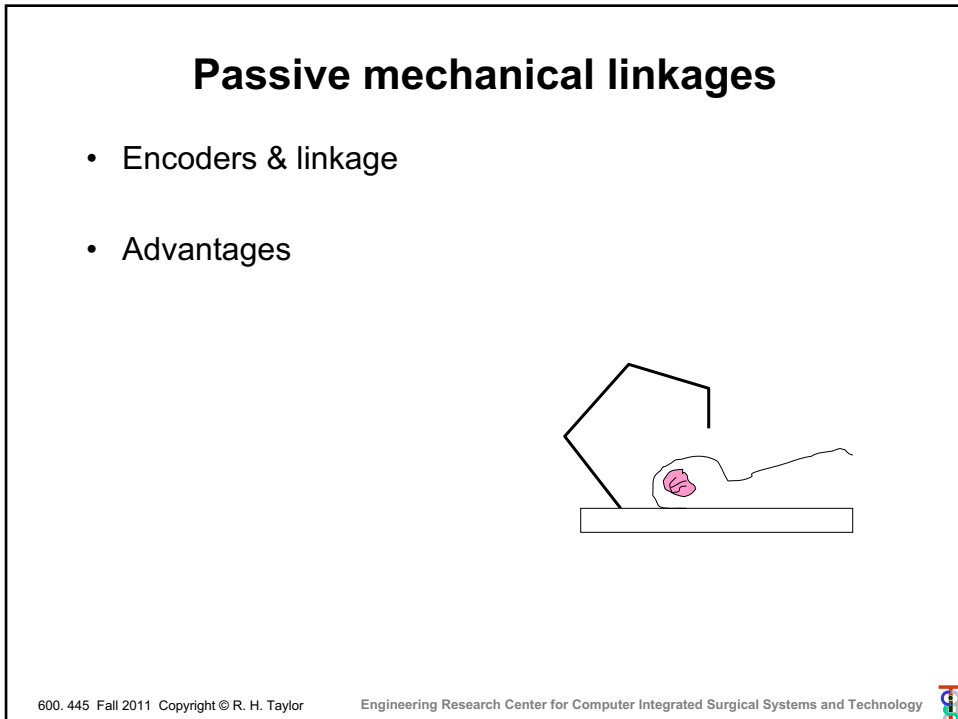


16



## Passive mechanical linkages

- Encoders & linkage
- Advantages:
  - simple
  - no line-of-sight problems



600. 445 Fall 2011 Copyright © R. H. Taylor


Engineering Research Center for Computer Integrated Surgical Systems and Technology



17

## Passive mechanical linkages

- Encoders & linkage
- Advantages:
  - simple
  - no line-of-sight problems
- Drawbacks
  - clumsy
  - single frame
  - reference base




600. 445 Fall 2011 Copyright © R. H. Taylor

Engineering Research Center for Computer Integrated Surgical Systems and Technology



18

## Some commercially used examples

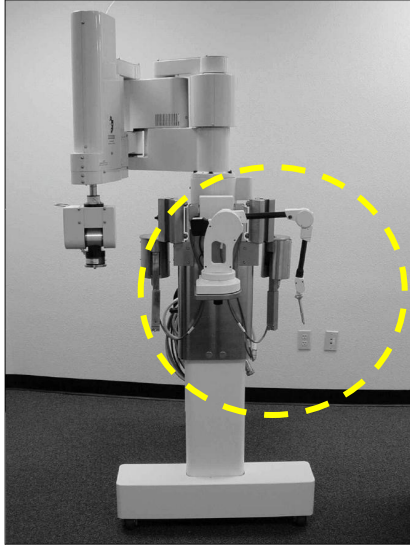

600. 445 Fall 2011 Copyright © R. H. Taylor



Engineering Research Center for Computer Integrated Surgical Systems and Technology



20

## Active mechanical linkages

- Robot + hand guiding
- E.g., Robodoc, REMS

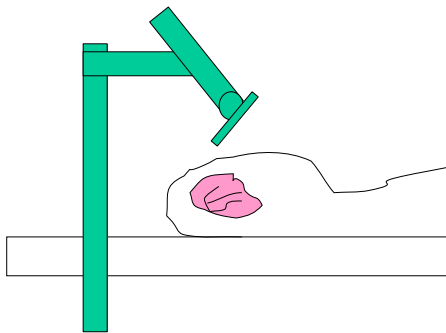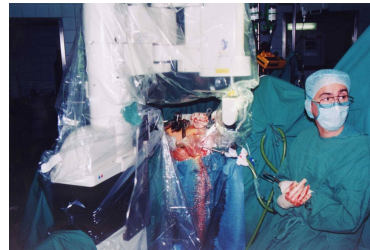

600. 445 Fall 2011 Copyright © R. H. Taylor


Engineering Research Center for Computer Integrated Surgical Systems and Technology



21

## Active mechanical linkages

- Robot + hand guiding
- E.g., Robodoc
- Advantages

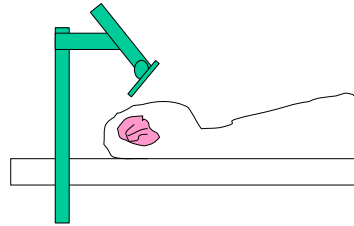

600. 445 Fall 2011 Copyright © R. H. Taylor


Engineering Research Center for Computer Integrated Surgical Systems and Technology



23

## Active mechanical linkages

- Robot + hand guiding
- E.g., Robodoc
- Advantages
  - accurate
  - registered to robot
  - can combine with search, actions
- Drawbacks

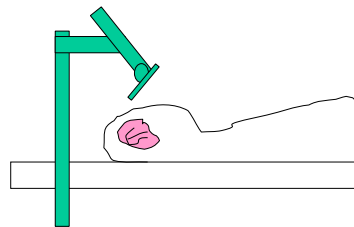

600. 445 Fall 2011 Copyright © R. H. Taylor


Engineering Research Center for Computer Integrated Surgical Systems and Technology



24

## Active mechanical linkages

- Robot + hand guiding
- E.g., Robodoc
- Advantages
  - accurate
  - registered to robot
  - can combine with search, actions
- Drawbacks
  - clumsy
  - expensive
  - single tool, referencing

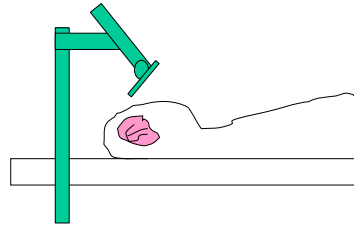

600. 445 Fall 2011 Copyright © R. H. Taylor


Engineering Research Center for Computer Integrated Surgical Systems and Technology



25

## Ultrasound

- “Clickers”+microphones
- time delays give distances
- multiple distances give pos.

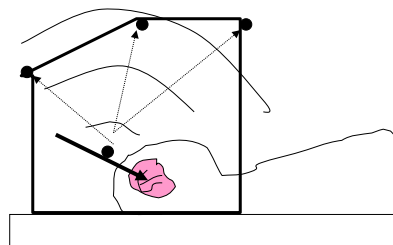

600. 445 Fall 2011 Copyright © R. H. Taylor

Engineering Research Center for Computer Integrated Surgical Systems and Technology



26

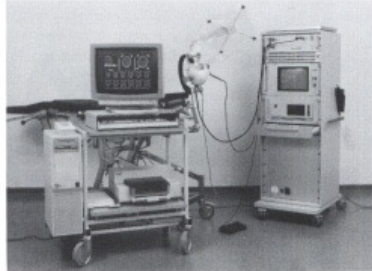


FIGURE 23.9 First sonic digitizer: system overview. Graphic computer (left), head-holder, sonic system (middle), SAC device, measuring computer (right).

intraoperative application. While we were evaluating the Science Accessories Corporation's (SAC) sonic system, we read about a first application of this device by Roberts [14] for the spatial, image-assisted localization of an operating microscope.

SONIC MICROSTEREOMETRY: ET-03

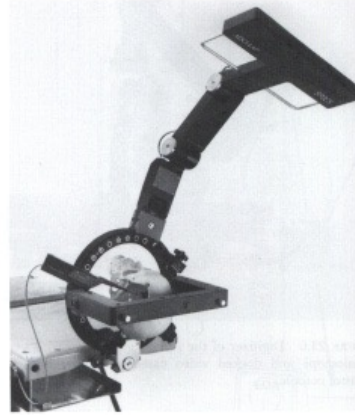


FIGURE 23.10 SPOCS with emitter panel (top), head-holder with detachable calibration frame, and supported targeting instrument (below left).

A Comparison of Sonic Digitizers Versus Light-Emitting Diode-Based Localization

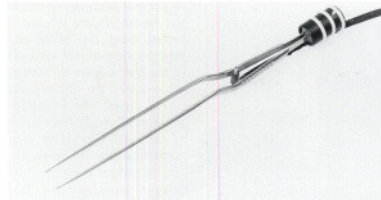


Figure 8. Sonic forceps, with wires directly attached to the emitters since the voltages involved precluded the use of a miniaturized connector.

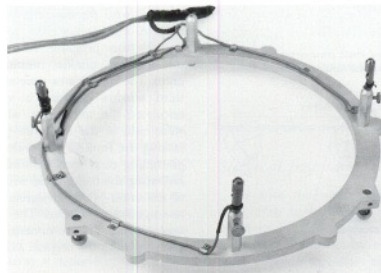


Figure 9. Sonic emitter ring, which attaches to the BRW head ring by the standard BRW ball/cam lock system; emitters can be placed at four points around the ring, allowing its use for posterior-based craniotomies.

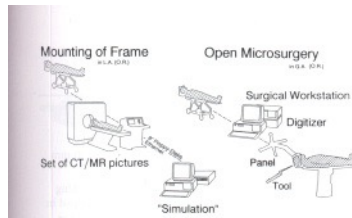


FIGURE 23.11 Sonic microstereometry. Data acquisition and operating procedure.

three microphones were docked with the ring at the same time, immediately after image data acquisition, or in a separate second procedure (see figure 23.11). The system was calibrated with a calibration panel containing three emitters, which were screwed temporarily to the ring. On the basis of the CT or MRI calibration marks, the software determines the exact position of each individual image relative to the calibration panel or base ring (first matrix operation) and then calculates the spatial relationship with the microphone panel (second matrix operation). The position of the targeting tool (one to four emitters) relative to the panel is determined finally in a third matrix operation.

The effect of interfering thermal factors could be largely eliminated by means of a measuring distance between the foot of the panel close to the head-retaining ring and the panel. Before each measuring cycle, a reference signal was emitted by the reference emitter and reached the panel microphones approximately 60 cm away in a known time of travel. Deviations (e.g., owing to temperature shifts) were taken into account auto-

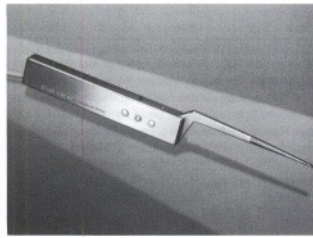


FIGURE 23.12 Bayonet-shaped standard measuring tool.


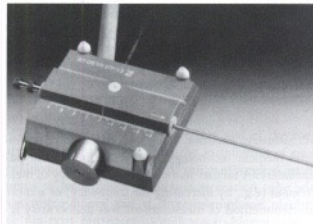


FIGURE 23.13 Measurement platform with four emitters for stereotaxy.




## Ultrasound

- “Clickers”+microphones
- time delays give distances
- multiple distances give pos.
- Advantages

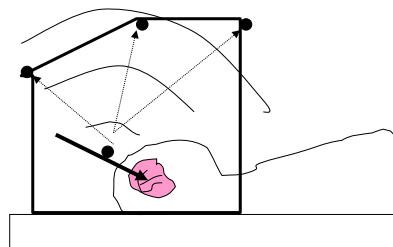

## Ultrasound


- “Clickers”+microphones
- time delays give distances
- multiple distances give pos.
- Advantages
  - Cheap, unobtrusive
  - multiple rigid bodies

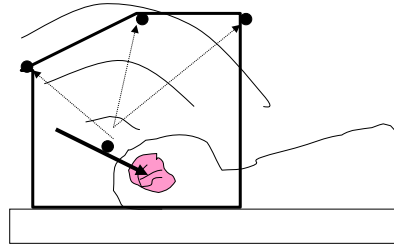

31

## Ultrasound


- “Clickers”+microphones
- time delays give distances
- multiple distances give pos.
- Advantages
  - Cheap, unobtrusive
  - multiple rigid bodies
- Drawbacks
  - Accuracy drifts (e.g., temperature)
  - Lack of self-evident warning

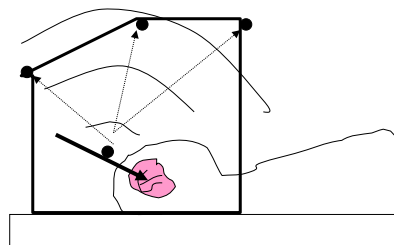

32


## Electromagnetic

- Originally developed for fighter pilot head tracking
- Reasonably accurate 6 dof
- E.g., Polhemus, Ascension, NDI Aurora
- Advantages
- Drawbacks

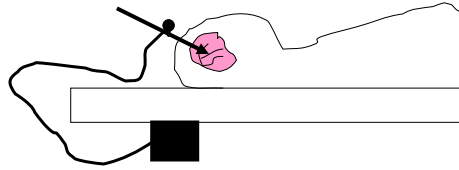

34

## How Does An EM System Work?

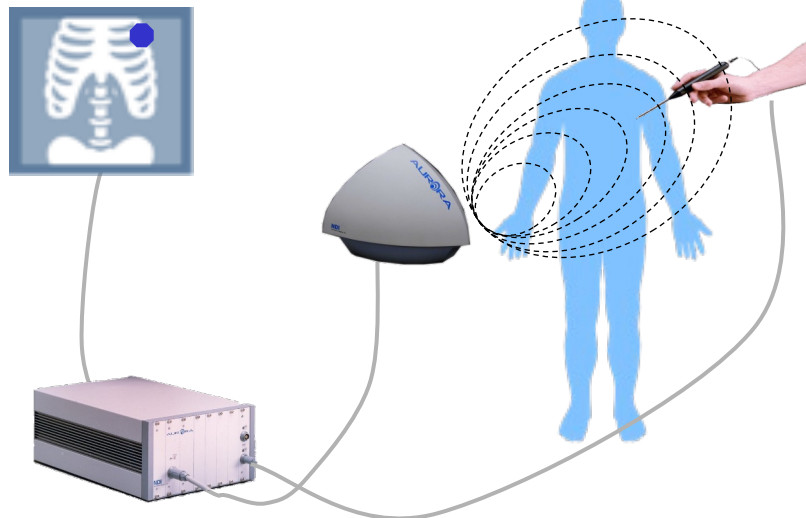

Credit: Paul McDonald, NDI




35




## How a Magnetic System Works

5D Sensor

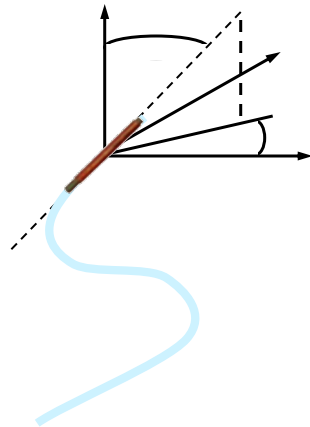

6D Reference

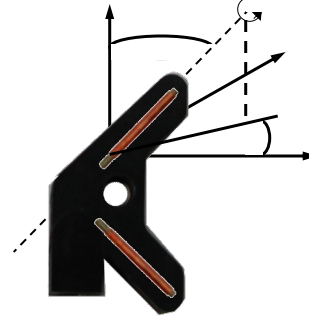

Credit: Paul McDonald, NDI

600. 445 Fall 2011 Copyright © R. H. Taylor

Engineering Research Center for Computer Integrated Surgical Systems and Technology

36

## Current Electromagnetic Products




NDI Aurora



SNT Axiem

Ascension Flock of Birds

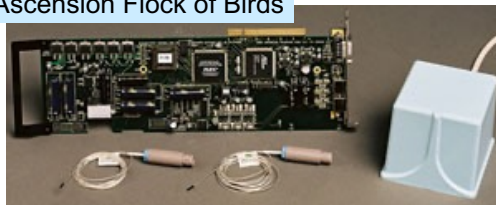

Polhemus Patriot

600. 445 Fall 2011 Copyright © R. H. Taylor

Engineering Research Center for Computer Integrated Surgical Systems and Technology

37

## Example: NDI Aurora™




Transmitter



5 DOF Sensors



6 DOF Sensors



<http://www.ndigital.com/medical/aurora-techspecs.php>

600. 445 Fall 2011 Copyright © R. H. Taylor





Engineering Research Center for Computer Integrated Surgical Systems and Technology



38

## Example: ATI medSAFE™ (Sensors)

### Sensor options:

<p><b>Model 90 6DOF Sensor</b></p> 	<p><b>Model 90 6DOF Sensor</b></p> <ul style="list-style-type: none"> <li>• Sensor OD = 0.9 mm</li> <li>• Sensor Length = 7.25 mm</li> <li>• Cable OD = 0.6 mm</li> <li>• Cable length = 6.6 ft. (2.0 m)</li> </ul>
<p><b>Model 130 6DOF Sensor</b></p> 	<p><b>Model 130 6DOF Sensor</b></p> <ul style="list-style-type: none"> <li>• Sensor OD = 1.5 mm</li> <li>• Sensor Length = 7.6 mm</li> <li>• Cable OD = 1.2 mm</li> <li>• Cable length = 6.6 ft. (2.0 m)</li> </ul>
<p><b>Model 180 6DOF Sensor</b></p> 	<p><b>Model 180 6DOF Sensor</b></p> <ul style="list-style-type: none"> <li>• Sensor OD = 2 mm</li> <li>• Sensor Length = 9.9 mm</li> <li>• Cable OD = 1.2 mm</li> <li>• Cable length = 6.6 ft. (2.0 m)</li> </ul>
<p><b>Model 800 6DOF Sensor</b></p> 	<p><b>Model 800 6DOF Sensor</b></p> <ul style="list-style-type: none"> <li>• Sensor OD = 7.9 mm</li> <li>• Sensor Length = 19.8 mm</li> <li>• Cable OD = 3.8 mm</li> <li>• Cable length = 6.6 ft. (2.0 m)</li> </ul>

<http://www.ascension-tech.com/medical/medSAFE.php>

600. 445 Fall 2011 Copyright © R. H. Taylor

Engineering Research Center for Computer Integrated Surgical Systems and Technology



39

## Example: ATI medSAFE™ (Transmitters)

### Transmitter options:

<p><b>Short-Range Transmitter</b></p>		<p><b>Set-Up &amp; Use:</b> 6.3 cm (2.5 inches) x 4.6 cm (1.8 inches) x 5.2 cm (2.1 inches). Transmitter weighs just 290 grams. It generates pulsed DC magnetic fields for high accuracy tracking in short-range applications.</p> <p><b>Ranges:</b></p> <ul style="list-style-type: none"> <li>• 46 cm for Model 800 Sensor; contact Ascension for performance of smaller sensors with this transmitter.</li> </ul>
<p><b>Mid-Range Transmitter</b></p>		<p><b>Set-Up &amp; Use:</b> 9.6 cm (3.8 inches) cube that generates pulsed DC magnetic fields for high accuracy tracking over medium ranges.</p> <p><b>Ranges:</b></p> <ul style="list-style-type: none"> <li>• 36 cm for Model 90 Sensor</li> <li>• 46 cm for Model 130 Sensor</li> <li>• 58 cm for Model 180 Sensor</li> <li>• 78 cm for Model 800 Sensor</li> </ul>
<p><b>Flat Transmitter</b></p>		<p><b>Set-Up &amp; Use:</b> 56 cm (22 inches) x 56 cm (22 inches) x 2.54 cm (1 inch). Flat transmitter is for unobtrusive placement beneath a patient. It generates a field above planar surface while negating any possible distortion of measurements by ferrous metal in an OR procedural table.</p> <p><b>Ranges:</b></p> <ul style="list-style-type: none"> <li>• 40 cm for Model 90 Sensor</li> <li>• 46 cm for Model 130 Sensor</li> <li>• 46 cm for Model 180 Sensor</li> <li>• 46 cm for Model 800 Sensor</li> </ul>

<http://www.ascension-tech.com/medical/medSAFE.php>

600. 445 Fall 2011 Copyright © R. H. Taylor

Engineering Research Center for Computer Integrated Surgical Systems and Technology



40

## Electromagnetic

### Pros

- No line of sight required
- Tools can be populated with small sensors
- Generally less expensive than optical

### Cons

- Metal Interference
- Less stable than optical
- Smaller measurement volume
- Incapable of tracking more than a few 6DOF tools

Credit: Paul McDonald, NDI

600. 445 Fall 2011 Copyright © R. H. Taylor


Engineering Research Center for Computer Integrated Surgical Systems and Technology



42

## Optical active


- Track LED markers
- Triangulate to locate 3D
- E.g.: Optotrak, Pixsys
- Current “gold standard”
  
- Advantages
  
- Disadvantages

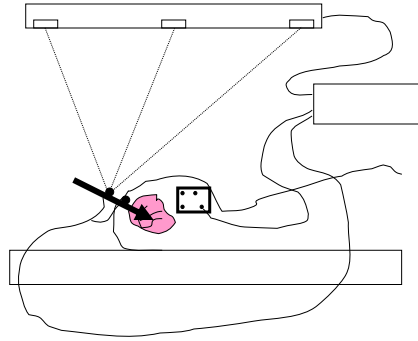

43

### A Comparison of Sonic Digitizers Versus Light-Emitting Diode-Based Localization

191

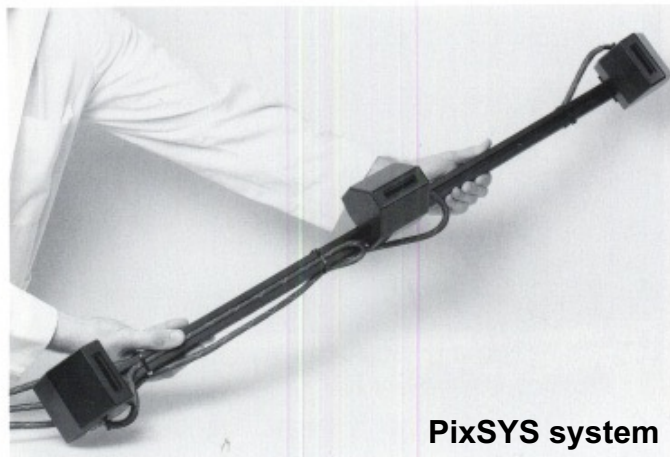

**PixSYS system**

*Figure 12. The optical camera system as implemented in the authors' system mounted on an aluminum extrusion.*



44

## Optical Active




600. 455/655 Fall 2022 Copyright R. H. Taylor

Engineering Research Center for Computer Integrated Surgical Systems and Technology



45

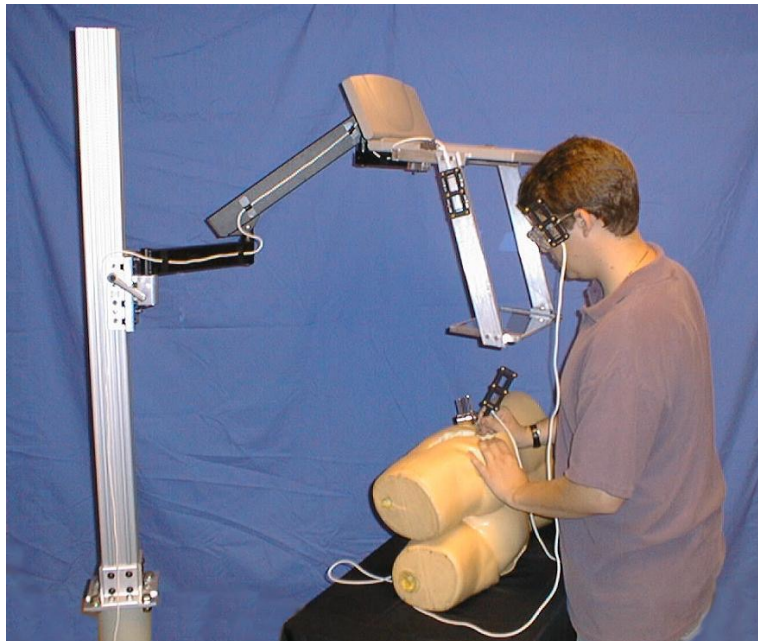

600. 455/655 Fall 2022 Copyright R. H. Taylor

Engineering Research Center for Computer Integrated Surgical Systems and Technology



46


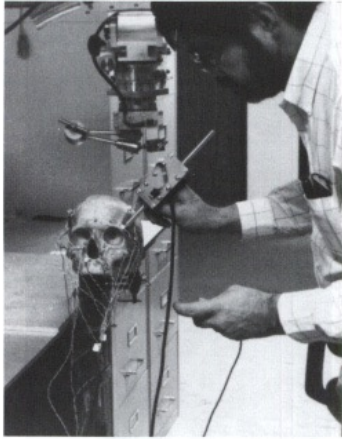


FIGURE 52.8 Locating landmarks on the skull. The position of the tip of the digitizer wand relative to the beacons on the wand has previously been calibrated. The positions of the beacons mounted to the skull are continuously monitored to provide a base coordinate system for the landmark location. Once the skull has been located, the positions of the beacons relative to the preoperative skull coordinate system may be computed.




## Optical active

- Track LED markers
- Triangulate to locate 3D
- E.g.: Optotrak, Pixsys
- Current “gold standard”
  
- Advantages

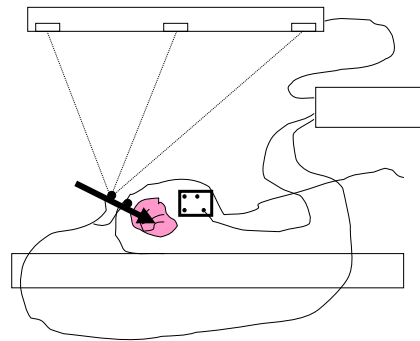

## Optical active

- Track LED markers
- Triangulate to locate 3D
- E.g.: Optotrak, Pixsys
- Current “gold standard”
- Advantages
  - very accurate
  - multiple rigid bodies
  - versatile
  - reasonably fail-safe
- Disadvantages

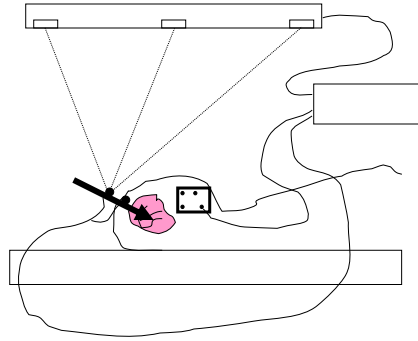

600. 455/655 Fall 2022 Copyright R. H. Taylor


Engineering Research Center for Computer Integrated Surgical Systems and Technology



49

## Optical active

- Track LED markers
- Triangulate to locate 3D
- E.g.: Optotrak, Pixsys
- Current “gold standard”
- Advantages
  - very accurate
  - multiple rigid bodies
  - versatile
  - reasonably fail-safe
- Disadvantages
  - line-of-sight restrictions
  - large, expensive

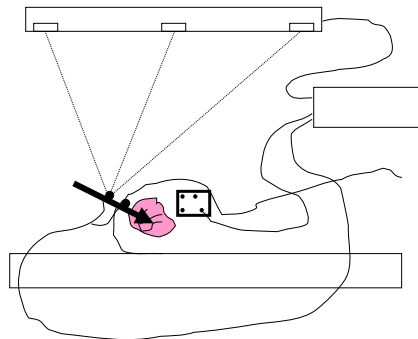

600. 445 Fall 2011 Copyright © R. H. Taylor


Engineering Research Center for Computer Integrated Surgical Systems and Technology



50

## Optical passive

- Triangulate markers in standard video images or specialized IR cameras
- E.g.,
  - Heilbrun, Colchester, Mathelin, ...
  - Polaris, Claron

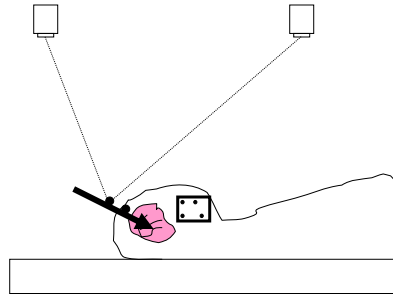

51



FIGURE 51.3 Optical position measurement for CAS.



52



## Commercial Example (Reflective Markers): NDI Polaris



600. 445 Fall 2011 Copyright © R. H. Taylor


Engineering Research Center for Computer Integrated Surgical Systems and Technology



53

## How does the Polaris system work?

The illuminators flood the area with infrared light

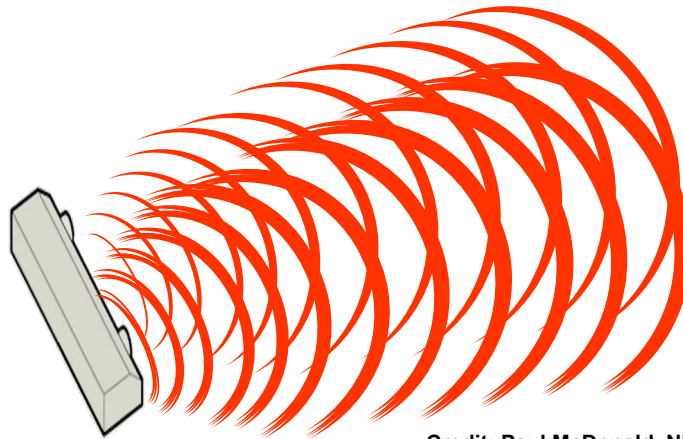

Credit: Paul McDonald, NDI

600. 445 Fall 2011 Copyright © R. H. Taylor

Engineering Research Center for Computer Integrated Surgical Systems and Technology




54

## How does the Polaris system work?

The infrared light is **reflected** back to the Position Sensor by the passive markers, while active markers **emit** infrared light.

By calculating the position of each individual marker on a tool, the System is able to determine the exact location of the tip of the tool using a pre-determined algorithm.

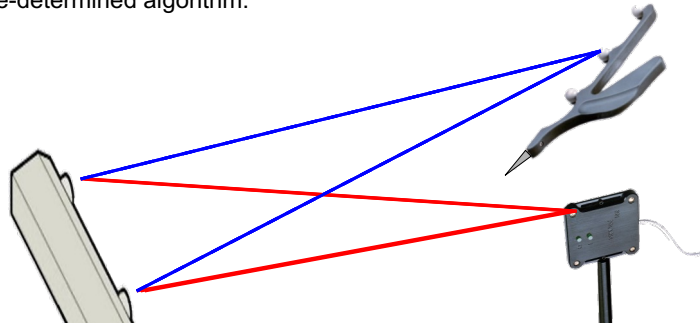

Credit: Paul McDonald, NDI

600. 445 Fall 2011 Copyright © R. H. Taylor

Engineering Research Center for Computer Integrated Surgical Systems and Technology



55

## Commercial Example (Ordinary Video): Claron Technology



<http://www.clarontech.com>



MicronTracker 2.1

Enhanced Reality:  
Tooltip feedback



MicronTracker 2.1

Enhanced Reality:  
3D Tracing


600. 445 Fall 2011 Copyright © R. H. Taylor

Engineering Research Center for Computer Integrated Surgical Systems and Technology





56

## JHU research examples: tool tracking

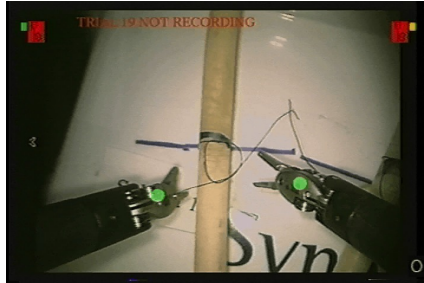

Track video of tools in mono or stereo images

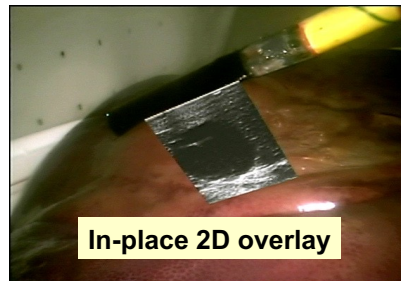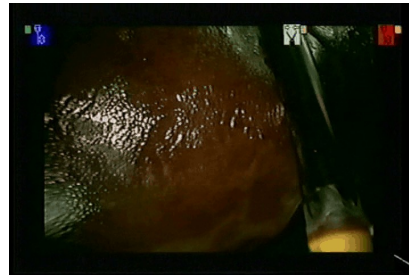

600. 445 Fall 2011 Copyright © R. H. Taylor


Engineering Research Center for Computer Integrated Surgical Systems and Technology



57

## Optical passive

- Triangulate markers in standard video images or specialized IR cameras
- E.g.,
  - Heilbrun, Colchester, Mathelin, ...
  - Polaris, Claron
- Advantages
  - Inherent alignment for overlay
  - Same method thru microscope
  - Standard components
  - Fairly fail-safe
- Drawbacks
  - More computing needed (but special hardware possible)
  - Line-of-sight
  - Video resolution

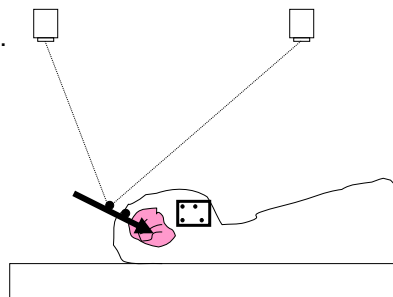

600. 445 Fall 2011 Copyright © R. H. Taylor

Engineering Research Center for Computer Integrated Surgical Systems and Technology



58

## Optical Summary

### Pros

- Industry Standard
- Well known and defined performance characteristics
- Ability to track large multiple of tools simultaneously
- Accuracy typically below 0.35 mm RMS
- Large measurement volume
- Variety of targets can be affixed to the tool (IRED, sphere)
- Video self alignment [rht]

### Cons

- Line-of-sight required
- Extraneous IR (sunlight)
- Rigid body tracking is most accurate, unable to track flexible devices
- Historically more costly when compared to other technologies
- Larger tools

**Credit: Paul McDonald, NDI**

