

Tracking and Characterization of Fragments in a Beating Heart using 3D Ultrasound for Interventional Guidance

Paul Thienphrapa^{1,2}, Bharat Ramachandran¹, Douglas Stanton¹, Haytham Elhawary¹, and Aleksandra Popovic¹

¹ Philips Research North America, Briarcliff Manor, NY, USA


² Johns Hopkins University, Baltimore, MD, USA

Abstract. Fragments generated by explosions and similar incidents can become trapped in a patient’s heart chambers, potentially causing disruption of cardiac function. The conventional approach to removing such foreign bodies is through open heart surgery, which comes with high peri-operative risk and long recovery times. We thus advocate a minimally invasive surgical approach through the use of 3D transesophageal echocardiography (TEE) and a flexible robotic end effector. In a phantom study, we use 3D TEE to track a foreign body in a beating heart, and propose a modified normalized cross-correlation method for improved accuracy and robustness of the tracking, with mean RMS errors of 2.3 mm. Motion analysis of the foreign body trajectory indicates very high speeds and accelerations, which render unfeasible a robotic retrieval method based on following the tracked trajectory. Instead, a probability map of the locus of the foreign body shows that the fragment tends to occupy only a small sub-volume of the ventricle, suggesting a retrieval strategy based on moving the robot end effector to the position with the highest spatial probability in order to maximize the possibility of capture.

1 Introduction

Penetration of a fragment into the heart is a common injury in both civilian accidents and military warfare [13], [15]. Small caliber bullets and small shell fragments with low velocity tend to circulate freely in the chambers, potentially leading to arrhythmia, occlusion, and possibly death [5], [12]. The most frequent treatment approach to removing these fragments involves open surgery via a median sternotomy [13] and cardiopulmonary bypass (CPB) [6], a highly invasive procedure requiring a long recovery period. Risks of this procedure include bacterial mediastinitis, hemolysis, blood clotting, and air embolism.

The long term objective of this work is to develop a flexible robotic system for minimally invasive retrieval of



fragments from a beating heart. A minimally invasive approach can significantly improve the management of cardiac fragments by reducing risk and mortality, improving postoperative recovery, and potentially reducing operating room times. The objectives of the present study are (1) to demonstrate the utility of 3D transesophageal echocardiography (TEE) in tracking a target moving rigorously against a dynamic background; (2) to develop real-time tracking of the fragments; and (3) to analyze its motion in the context of a robotic retrieval system.

The use of 3D ultrasound for interventional systems is a fairly recent development due to high cost, low resolution, and inability to access real-time data streams [3]. In [11], markers were attached to an instrument to allow for image-based tracking. Variability in the readings was less than 1 mm. The instrument was subsequently driven towards targets in a water tank, reaching them with an error of 1.2 mm [7]. In a step towards clinical conditions, targets were embedded in turkey breast in [4] and were reached in all five trials. Experiments with low-resolution 3D catheter transducers [14] yielded errors of approximately 3 mm. However, the targets were static in these experiments.

Ferrous shrapnel can be difficult to detect in ultrasound when adjacent to other hyperechoic surfaces. In [9], a variable magnetic field is used to induce vibrations in shrapnel, thus illuminating it under color flow Doppler and allowing it to be located within an error of 1.06 mm.

The performance requirements for tracking a foreign body in the heart are more akin to the 1-degree-of-freedom (DOF) heartbeat compensation devices of [1], [16]. Predictive control was employed to track heart structures in one dimension with positive results. On the other hand, cardiac motions are more predictable than that of an object moving freely within the heart. Due to a variety of influences, foreign bodies are prone to seemingly arbitrary motions. A predictive control scheme is less likely to be effective in this case. The main contribution of this paper is the tracking of an unpredictably moving target using 3D TEE, for the purpose of developing a retrieval strategy by a flexible robotic device inserted through the apex of the heart.

2 Experimental Setup

A system for studying the problem of minimally invasive evacuation of fragments from a beating heart is illustrated in Fig. 1. It includes an ultrasound system, a beating heart phantom, and a workstation (2.3 GHz Intel Xeon, 4 GB of RAM) that acquires live streaming ultrasound volumes over TCP/IP.

The Philips iE33 xMATRIX Echocardiography System is used with the X7-2t 3D TEE probe. Each image has a resolution of $128 \times 48 \times 112$ voxels of size 0.81, 0.96, and 0.98 mm, spanning a field of view of 60° azimuth, 30° elevation, and 12 cm depth respectively. Gain and compression are set at 47% and 40 dB.

The beating heart phantom is a custom developed multi-modality phantom compatible with X-ray, ultrasound, and MR imaging. Made of polyvinyl acetate (PVA), it is a full replica of a human heart and resides in an acrylic glass water

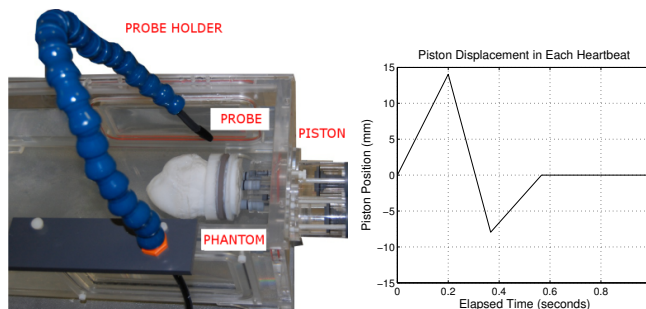


Fig. 1. (Left) Arrangement of the TEE probe and the heart phantom. (Right) Piston displacement in the beating heart phantom for one heartbeat.

tank. Two servo-actuated pneumatic pistons pump water into and out of the phantom to create the deformable effect of a heartbeat and blood flow. Each piston pumps about 18 ml of water per heartbeat; its motion is given in Fig. 1. The stroke volume is chosen to be lower than in healthy humans to mimic both surgical [10] and cardiovascular conditions following heart injury. For these experiments the heart rate was set at 1 Hz.

A 3.2 mm steel ball was selected to act as a fragment due to its likeness to the clinical case in terms of size (typically 2-5 mm) and material. The fragment was imaged under 3D TEE at 20 frames per second (fps) and manually segmented from five datasets ($n=5$) of 400 frames (20 seconds) each. This duration was empirically found to capture most of the activity that would occur in a given trial. Furthermore, 20 heart cycles are sufficient for testing of online tracking methods and their robustness—a previous study reports on an *in vivo* instrument tracking experiment with a beating heart using a five-second window [8]. Fig. 2 shows an example of the foreign body in the heart phantom after manual identification in the 3D TEE image.

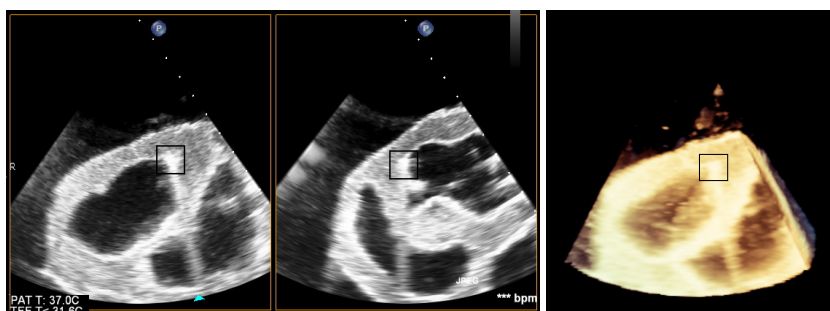


Fig. 2. (Left and center) Orthogonal slices showing the fragment (outlined) in the right ventricle of the heart phantom. (Right) A three-dimensional view.

3 Real-Time Tracking of the Fragment

3.1 Approach

Normalized cross-correlation (NCC) is a well-known template-matching algorithm commonly used in image processing applications to search for desired features. The correlation coefficient at a voxel, $R(u, v, w)$, for a template $t(x, y, z)$ is given in (1). Normalization, accomplished by subtracting the mean from the template and the image under the template (\bar{t} and \bar{f} respectively) and dividing by their standard deviations, provides for robustness against variations in intensity, which can occur as both the fragment and background move around.

$$R(u, v, w) = \frac{\sum_{x,y,z} [f(x, y, z) - \bar{f}] [t(x - u, y - v, z - w) - \bar{t}]}{\sqrt{\sum_{x,y,z} [f(x, y, z) - \bar{f}]^2 \sum_{x,y,z} [t(x - u, y - v, z - w) - \bar{t}]^2}} \quad (1)$$

The fragment was selected interactively from the first image frame to define the template for the algorithm to track in subsequent frames. A template of size $10 \times 10 \times 10$ voxels was suitable for enclosing the entire fragment, while a search space of $40 \times 30 \times 30$ was sufficient to capture displacements between frames. The low computation time of NCC (38 ms per frame) means it is especially suited for tracking within a system where near real-time performance is required.

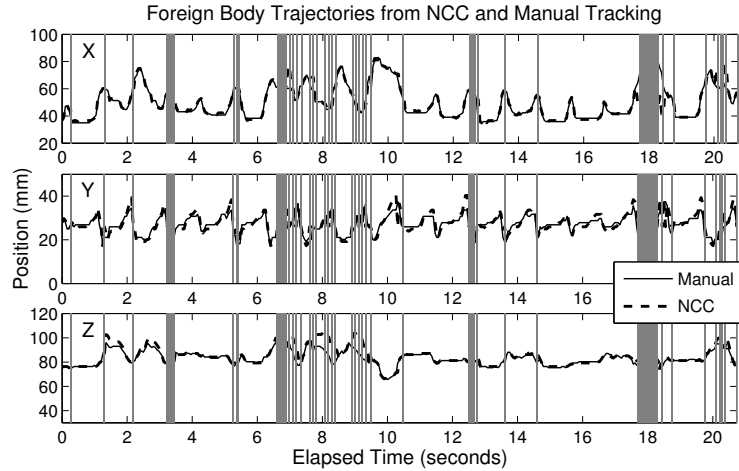


Fig. 3. Fragment trajectories based on NCC vs. manual tracking. Dropped frames are marked by vertical lines.

The coefficient R in (1) is a real number in $[-1, 1]$, with higher values indicating a close match and values tending toward -1 signifying an inverted match. The location of the maximum R (R_{max}) found in a search space is taken to be

the position of the fragment. However, a weakness of NCC is that it relies on consistency in the appearance of the target, whereas appearances may vary in ultrasound due to noise, artifacts, and low resolution. This can lead to the target being incorrectly identified in some frames. A low R_{max} suggests that NCC was not confident in its decision, and errant tracking can be avoided by ignoring such frames. In our experiments, a frame i is dropped if $R_{i,max}$ is less than c standard deviations below the mean of the dataset. The value of c can be tuned to the level of confidence desired; we found $c=0.9$ to exhibit a reasonable compromise between spatial and temporal accuracy.

$$R_{i,max} < R_{mean} - c \cdot R_{sd} \quad (2)$$

3.2 Results

Accuracy. Fig. 3 shows a trace of the fragment as determined by NCC, with manually-segmented fragment localization serving as a basis for evaluation.³ Table 1 lists the number of dropped frames and accuracy for all datasets. NCC-based fragment tracking with detection of low confidence intervals (post-drop error) was accurate to within 2.3 mm rms after dropping 18.5% of frames. As expected, in the case of NCC without frame dropping (pre-drop error), tracking was lost in some frames resulting in mean errors that were almost twice as high (4.3 mm). For frames in which the reported fragment location is unavailable or doubtful, it is preferable to have the system wait until tracking is recovered, allowing the robotic retrieval instrument to stay in its current position or to be placed at a safe location if the uncertainty is prolonged over several frames.

Table 1. Performance of NCC vs. manual tracking.

Parameter	Datasets					Aggregate			
	1	2	3	4	5	Min	Mean	Max	SD
Pre-Drop Error (mm rms)	6.2	4.8	5.3	2.5	2.6	2.5	4.3	6.2	1.7
Post-Drop Error (mm rms)	2.0	3.1	2.6	1.8	2.1	1.8	2.3	3.1	0.5
% Frames Dropped	20.9	15.5	20.1	22.9	13.3	13.3	18.5	22.9	4.0
$100 \times R_{mean}$	80.4	71.0	83.6	85.1	84.0	71.0	80.8	85.1	5.8
$100 \times R_{sd}$	9.2	8.5	10.3	4.8	3.7	3.7	7.3	10.3	2.9

Motion Characterization. Table 2 summarizes the extracted motion parameters. The average range of motion is 40.2 mm over three axes. While there is some correspondence between fragment motion and heartbeats (see Fig. 3), there is an element of arbitrary motion as well. Frequency domain analysis (Fig. 4) supports this observation with the primary peak located at 1 Hz, but with spectral

³ Video posted at <http://www.youtube.com/watch?v=u-KYpbS33-8>.

power at both lower and higher frequencies suggesting a more complex behavior. Previous studies have found higher frequency components in the mitral valve as well [16].

Table 2. Fragment motion parameters obtained from 3D TEE images.

Parameter	Datasets					Aggregate			
	1	2	3	4	5	Min	Mean	Max	SD
Range (mm)	51.4	49.0	47.5	23.5	29.8	23.5	40.2	51.4	12.7
Speed (mm/s)	336.2	334.2	530.0	208.7	308.3	208.7	343.5	530.0	116.5
Accel. (m/s^2)	5.3	9.5	9.1	6.2	8.7	5.3	7.8	9.5	1.9

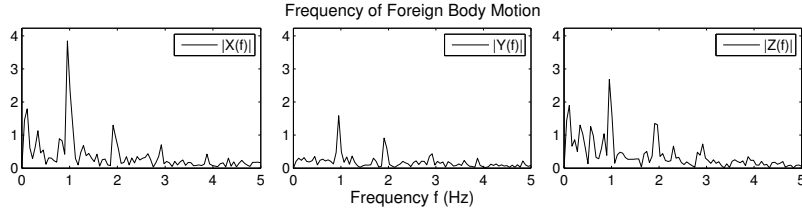


Fig. 4. Frequency components of fragment motion.

The fragment reaches speeds of about 343.5 mm/s. Similar speeds have been reported for the heart wall (300 mm/s [2]) and mitral valve (200 mm/s [16]). Acceleration (7.8 m/s^2 on average) is higher than figures reported for the mitral valve (3.8 m/s^2 [16]). A retrieval strategy based on following the trajectory of the foreign body using a robotic end effector would be extremely challenging given these high speeds and accelerations. Furthermore, the uncertainties inherent in a beating heart environment may make it hazardous to do so. We thus propose a different approach for retrieval of the foreign body, wherein the real-time tracking method described in this paper is used to build a spatial probability map of the fragment, based on its past locations. The map can then be used to position a dexterous robotic device in the most visited locations of the fragment in order to maximize the possibility of capture.

4 Probability Map

A qualitative representation of the fragment motion, generated using the tracking approach described above, is shown in Fig. 5. Warmer (red) regions indicate where the fragment is more likely to be located based on fragment traces. The apparent tendency of the fragment to be localized in a subsection of the overall

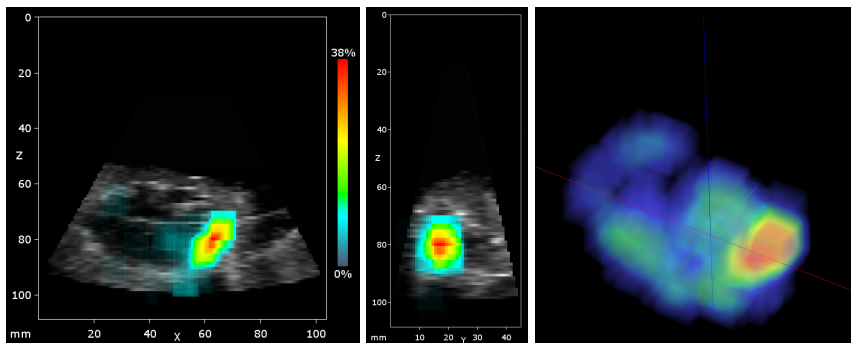


Fig. 5. Probability map of the fragment position. (*Left and center*) Coronal and sagittal slices of the map. (*Right*) Three-dimensional view.

ventricular volume suggests the viability of a more relaxed retrieval approach based on aiming the dexterous robotic end effector at the volume of highest probability of fragment location. Histograms (Fig. 6 and Table 3) show that on the average across datasets, the fragment spends up to 50.5% of the time in the most visited voxel. Although it is shown in the frequency domain (Fig. 4) that the motion of the fragment is more irregular than the motion of the heart wall, predictive models using the spatial position of the fragment can be used to move the robot to a ‘waiting’ position, i.e. the position with the highest spatial probability.

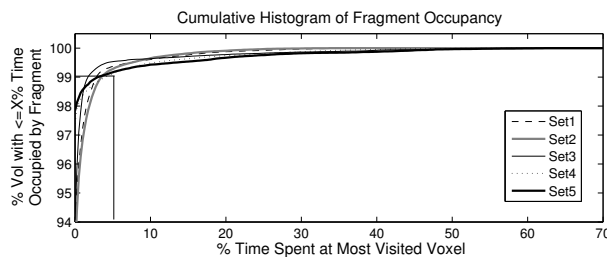


Fig. 6. Cumulative histograms showing how frequently voxels are visited by the fragment. Around $Y=94\%$ of the volume is never touched ($X=0\%$), and roughly $Y=99\%$ of the volume is occupied at most $X=5\%$ of the time.

5 Conclusions and Future Work

In this paper, the motion of a fragment in a beating heart phantom is quantified using motion tracking in 3D TEE images. We show that the fragment motion is fast, abrupt, and often unpredictable. This provides valuable insight regarding

Table 3. Tendency of fragment to visit certain locations. The first row describes the percentage of the volume occupied at least 25% of the time. The second lists the maximum percentage of time that any one voxel was occupied.

Parameter	Datasets					Aggregate			
	1	2	3	4	5	Min	Mean	Max	SD
25% FB Occupancy	0.07	0.03	0.17	0.19	0.24	0.03	0.14	0.24	0.09
Max Occupancy Level	39.8	38.0	57.5	54.0	63.0	38.0	50.5	63.0	11.1

the design of an interventional system that is capable of catching the particle. The next milestone will involve the design of robot control scheme that uses the spatial probability map of the foreign body location to safely retrieve the fragment.

References

1. Kesner, S., Yuen, S.G., Howe, R.D.: Ultrasound servoing of catheters for beating heart valve repair. In: *Int. Conf. on Info. Proc. in Computer-Assisted Interventions*. pp. 168–178 (2010)
2. Kostis, J.B., Mavrogeorgis, E., Slater, A., Bellet, S.: Use of a range-gated, pulsed ultrasonic Doppler technique for continuous measurement of velocity of the posterior heart wall. *Chest* 62(5), 597 (1972)
3. Krupa, A., Fichtinger, G., Hager, G.D.: Real-time motion stabilization with B-mode ultrasound using image speckle information and visual servoing. *Int. J. Robot. Res.* 28(10), 1334–1354 (2009)
4. Liang, K., Allmen, D.V., Rogers, A.J., Light, E.D., Smith, S.W.: Three-dimensional ultrasound guidance of autonomous robotic breast biopsy: feasibility study. *Ultrasound Med. Biol.* 36(1), 173–7 (2010)
5. Marshall, A.J., Ring, N.J., Newman, P.L.: An unexplained foreign body in the myocardium. *J. Royal Soc. Med.* 95, 250–251 (2002)
6. Nessen, S.C., Lounsbury, D.E.: *War Surgery in Afghanistan and Iraq: A Series of Cases, 2003-2007*, s.l. Department of the Army, Office of the Surgeon General and Borden Institute, 14: Thoracic Trauma (2008)
7. Novotny, P.M., Stoll, J.A., Dupont, P.E., Howe, R.D.: Real-time visual servoing of a robot using three-dimensional ultrasound. In: *IEEE Int. Conf. on Robotics and Automation*. pp. 2655–2660 (2007)
8. Novotny, P.M., Stoll, J.A., Vasilyev, N.V., del Nido, P.J., Dupont, P.E., Zickler, T.E., Howe, R.D.: GPU-based real-time instrument tracking with three-dimensional ultrasound. *Med. Image Anal.* 11, 458–464 (2007)
9. Rogers, A.J., Light, E.D., Smith, S.W.: 3-D ultrasound guidance of autonomous robot for location of ferrous shrapnel. *IEEE Trans. Ultrason., Ferroelectr., Freq. Control* 56(7), 1301–3 (2009)
10. Ryan, K.L., Cooke, W.H., Rickards, C.A., Lurie, K.G., Convertino, V.A.: Breathing through an inspiratory threshold device improves stroke volume during central hypovolemia in humans. *J. Appl. Physiol.* 104(5), 1402–9 (2008)
11. Stoll, J.A., Novotny, P.M., Howe, R.D., Dupont, P.E.: Real-time 3D ultrasound-based servoing of a surgical instrument. In: *IEEE Int. Conf. on Robotics and Automation*. pp. 613–618 (2006)

12. Symbas, P.N., et al.: Cardiac missiles: a review of the literature and personal experience. *Ann. Surg.* 211, 639–47 and 647–8 (1990)
13. United States Department of Defense: *Emergency War Surgery: Third United States Revision*, s.l., 16: Thoracic Injuries (2004)
14. Whitman, J., Fronheiser, M.P., Smith, S.W.: 3-D ultrasound guidance of surgical robotics using catheter transducers: feasibility study. *IEEE Trans. Ultrason., Ferroelectr., Freq. Control* 55(5), 1143–5 (2008)
15. Williams, J.C., Elkington, W.C.: Slow progressing cardiac complications—a case report. *J. Chiropr. Med.* 7, 28–33 (2008)
16. Yuen, S.G., Kettler, D.T., Novotny, P.M., Plowes, R.D., Howe, R.D.: Robotic motion compensation for beating heart intracardiac surgery. *Int. J. Robot. Res.* 28(10), 1355–1372 (2009)